

# L722 STACK PROBE

## INSTRUCTION MANUAL



**WAGNER  
METERS**  
Unleash Your Expertise

# TABLE OF CONTENTS

L722 Stack Probe Attachment	03
L722 Specifications	03
L722 Calibration	03
L722 Operation	04
Maintaining Accuracy Of Moisture Content Readings	04
L722 Maintenance	06
Cleaning	06
Spring Replacement	07
Hinge Repair/Replacement	07
Storage	08
Coil Cord Replacement	09
Repair Service	11
Warnings	14

## L722 Stack Probe Attachment

---

The Model L722 Stack Probe attachment, coupled with the L5300 (latest version) Industrial Handheld Wood Moisture Meter makes it easy to reach deep into stickered units of lumber and take accurate moisture readings without the danger of broken pins. Wagner's wood-friendly electromagnetic wave technology makes it possible to take multiple readings throughout an entire stack in just minutes.

**NOTE:** The L722 will work with either the L612, L622, or the L5300. For the remainder of this manual, the L5300 will only be referenced.

Once the probe is inserted between the boards, the springs press the end-mounted sensor flat against the wood to ensure deep penetration of the electromagnetic field. Then slide the probe slowly out of the stack, reading the moisture in each board as the sensor passes over it. Virtually unaffected by surface moisture, the L722 gives consistent and reliable readings in or out of kilns.

### L722 Specifications

---

<b>Physical Size: Overall Size Including Handle:</b>	L722L - L 48in x W 6.0in x H 1.625 in (121.9cm x 15.2cm x 4.12cm) L722S - L34in x W 6.0in x H 1.625 in (86.3cm x 15.2cm x 4.12cm)
<b>Probe Reach:</b>	L722L - L 40.5in (102.8cm) L722S - L 26.75in (67.9cm)
<b>Extrusion and Sensor Head:</b>	0.5in (12.7mm) thickness
<b>Min/Max Sticker Range:</b>	0.5in - 0.9in (12.7mm - 22.9mm)
<b>Scanning Area:</b>	2.5in x 2.5in (6.35cm x 6.35cm)
<b>Scanning Depth:</b>	1.0in (2.54cm) minimum
<b>Shipping Weight:</b>	L722L - 128 oz. (3.64kg) L722S - 112 oz. (3.18kg)

### L722 Calibration

---

Calibration is factory set. Calibration may be checked by using the On Demand Calibration Block (ODC) (included with the L5300), and following the instructions in the L5300 Manual. The probe calibration is verified in the same manner as the L5300 (Refer to the L5300 Owner's Manual).

## L722 Operations

---

To connect a probe to the L5300, remove the dust plug from the black-colored port on the right hand side of the meter and plug the connecting cable into this port.

With the probe connected to the L5300 and the meter ON, insert the probe into the sticker space between the layers of boards in a stack of lumber. The springs press the end-mounted sensor flat against the wood. The actual sensing area of the probe is located in the end of the probe assembly on the opposite side of the springs. Be sure to insert and remove the probe straight in and straight out of the stack of lumber to avoid damage to the L722 springs and hinge.

When the probe is connected to the meter, the internal hand-meter sensor is bypassed and the probe will be the source of the readings. The backlight will also be turned on automatically for easier viewing in the dark kiln environment.

## Maintaining Accuracy Of Moisture Content Readings

---

The purpose of this section is to provide proper moisture content measurement techniques during kiln drying operations. The major factor of preserving consistent readings is to control the many variables that are present when moisture content (MC) values are measured. The control of these variables will be identified and addressed in the following paragraphs.

**Taking L722 Stack Probe Measurements** – The L5300 meter should be checked for general operation and battery condition. Ensure the L5300 meter has been set for the appropriate wood species being measured.

Consistent use of the stack probe will maintain the integrity of MC readings. Ensure the sensor plate area is completely covered by the lumber being measured. Take several measurements with the probe oriented perpendicular to the lengths of the lumber. Measure close to the stickers as wood surfaces will be more uniform from board surface to board surface and less chance that the probe head will get caught on warped boards hanging down between the location of each sticker.

To avoid hinge damage, don't pull down on the probe handle.

Your kiln drying operations procedure should spell out the specific number of measurements to take, at what heights, at what depths in the stack to measure, and when to measure them in the drying cycle. In order to maintain consistency, take readings in the same locations in the stack, and at the same times in the drying cycle from one kiln charge to the next. You should take enough readings to be statistically significant. The more readings you take, the more accurate your average will be.

When taking measurements using a stack probe, you will be measuring the selected locations in the stack as stated in your kiln drying operations procedure. This will be the average moisture content of the scan area being measured directly under the sensor plate.

Keep in mind that the scan area of the L722 stack probe is 2.5" square (6.35cm) by 1" deep (2.54cm). This varies greatly from an in-line system, which has a much wider scan area (up to 12" square, 30.5cm), and deeper penetration. This will cause a larger area to be averaged with an in-line system.

The L722 stack probe readings will read excessively high when measuring severely knotted lumber due to higher density. Readings that are lower than the average readings taken are most likely due to measuring air gaps between boards or wane along the board edges.

## **Kiln Drying, Moisture Gradients, and Temperature**

---

Warm lumber tends to lose moisture after it is removed from the kiln and it continues to dry. The moisture content of kiln-dried lumber is typically higher in the center core and drier toward the ends and outer surfaces. Planing the drier top and bottom sections of a board will cause the MC value to be higher. Because it is difficult to control all of these elements, it is best to try to maintain consistency in storage, and apply a correction factor as discussed in the paragraph below.

**Applying Correction Factors** - Due to variances beyond the control of the user, the MC values obtained from kiln dried lumber as read from the hand meter/stack probe combination will likely not be exactly the same as read by an in-line system. An effective method to compensate for this is to establish a correction factor based on the nominal readings obtained in the kiln and the desired (target) MC reading, as seen at the In-line meter.

**You should be looking for a correlation between the stack probe readings and the in-line readings.**

Example: Packs 3, 7, 10, and 12 of 2x4 Douglas Fir are measured in a kiln by taking 50 readings in each pack after 20 hours of drying. The hot check average was 18%. That means the MC of this lumber going through the planer three days later will have a 16.5% average.

Use the stack probe MC as a reference and adjust your correction factor as necessary to obtain the desired target MC at the in-line console. Compile data from previous kiln cycles to fine-tune your correction factor.

Consistency is the key! If your process changes, consider the impact to your correction factor, but do everything possible to control the variables. Don't complicate the variables by measuring one way this time and another way the next.

If your consistent correction factor suddenly stops working, ask these questions: What has changed? Were the hot check readings taken the same way? Did the lumber have more MC variability going into the kiln? Did the meter recently get calibrated? Did the pack coming out of the kiln go through the planer sooner or later than usual?

Temperature can also have a small effect on the readings. High lumber temperatures can cause the MC reading to increase by 2-3%. These variances are far smaller than would be seen with a resistive pin meter. Some of this temperature-related measurement error could be attributed to the warm lumber losing moisture as it cools.

Try to measure the lumber at approximately the same temperature from one cycle to the next to maintain the best consistency in your readings. If possible, let the wood cool for a couple of hours prior to measurement. The temperature effect is small, and correlation is the real goal, but more accuracy can be obtained by letting the temperature stabilize.

## L722 Maintenance


---

### CLEANING

Maintenance of the probe consists of cleaning the probe assembly periodically with mild detergent or cleaning solution and a soft rag. Do not soak or submerge the probe in liquid. Scrape off excess pitch with a flat bladed instrument such as a chisel or putty knife, being careful not to dig into the probe. Never use solvent of any kind for cleaning.

### SPRING REPLACEMENT


When cleaning under the springs, remove the springs. **NEVER** lift up on the springs, as this will distort the metal. If the springs should become damaged in any way, replace them in pairs. See *Replacement Parts* section for Part Numbers, which may be purchased from the factory or through your distributor.

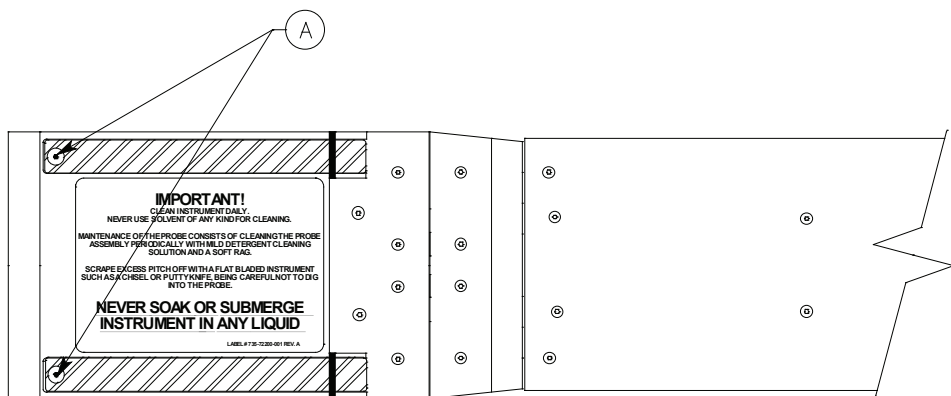

Symbol	Description
A	REMOVE SCREWS. REPLACE SPRINGS.

## HINGE REPAIR/REPLACEMENT

If the hinge becomes stretched, removal of the hinge screws and reseating of the hinge is all that is normally necessary. (Waiting for 30 minutes with the hinge removed will allow the hinge material to relax.) If the hinge is severely distorted, see *Replacement Parts* section for Part Numbers, which may be purchased from the factory or through your distributor.

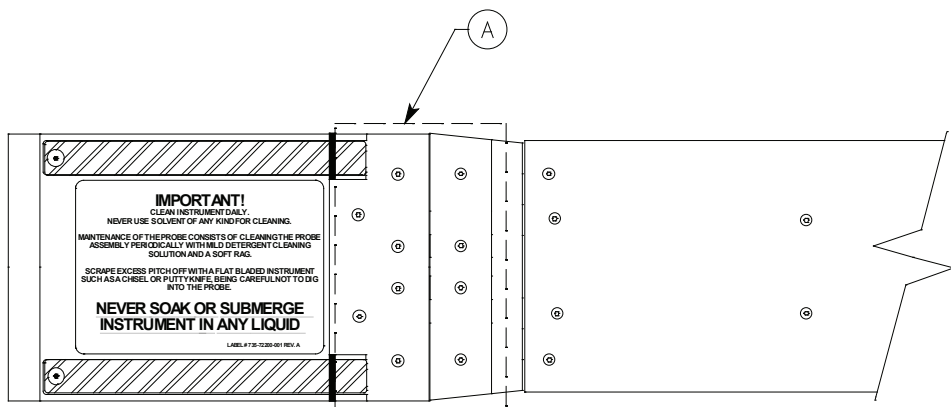

Symbol	Description
A	REMOVE HINGE SCREWS, AND RESEAT OR REPLACE HINGE.

# STORAGE


The stack probe should be cleaned and stored in a cool, dry environment.

## COIL CORD REPLACEMENT


**IF THE COIL CORD BECOMES DAMAGED, IT CAN BE REPLACED AS DESCRIBED BELOW:**

- Step 1:** Lay the L722 Stack Probe on a flat work space with the coil cord facing upward. Remove the 6 screws fastening the handle half-shells together. Separate the two halves of the handle.

Remove 6 handle screws

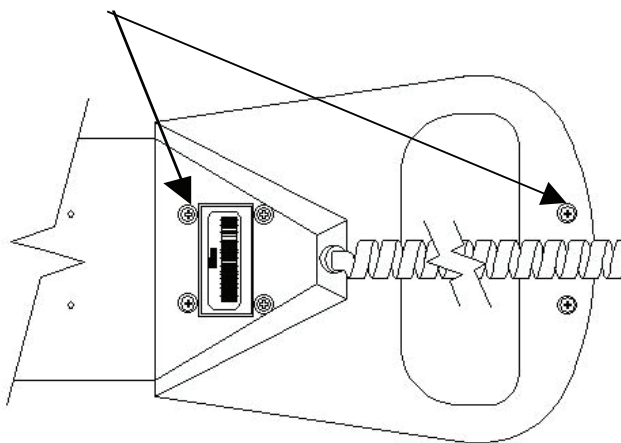


- Step 2.** Disconnect the old cord from the coupler.  
Depress lever and extract plug from coupler.

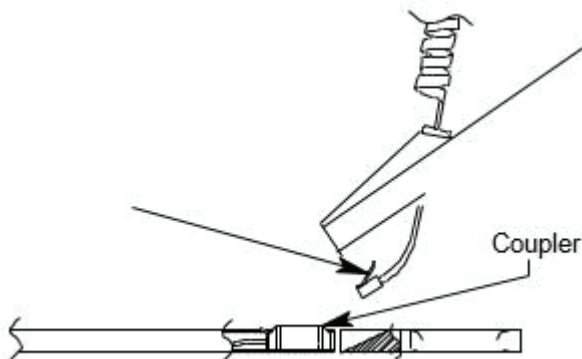



- **Step 3.** Remove the old cord from the handle half-shell.


Rotate strain relief so latch is accessible, then depress with screwdriver.

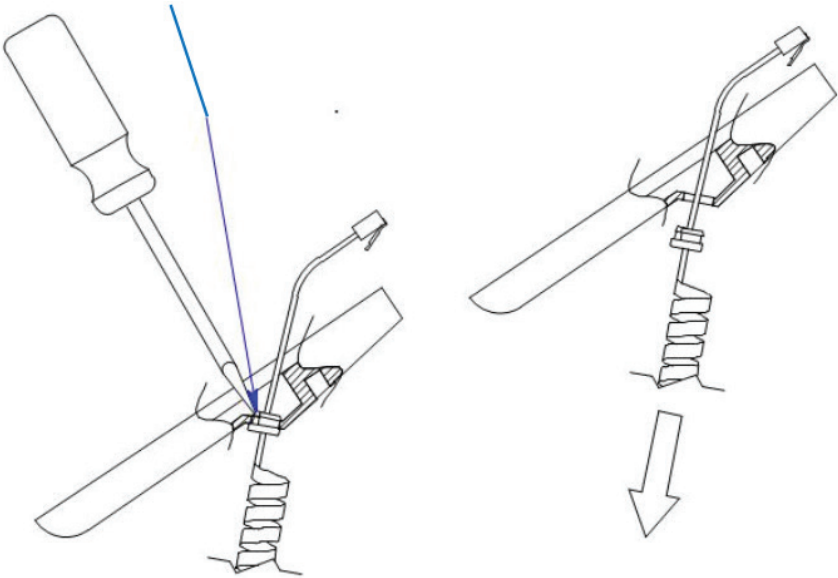


- **Step 4.** Install replacement cord.

Reuse the strain relief from old cord and insert until latch clicks into hole.


Extend the cord 3.75 inches into the handle half that has the offset connector on the outside of the stack probe.

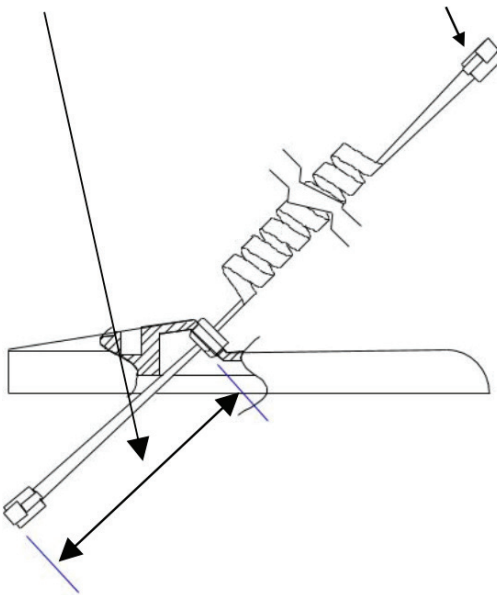

- **Step 5.** Connect replacement cord to coupler. Ensure latch clicks into detent.

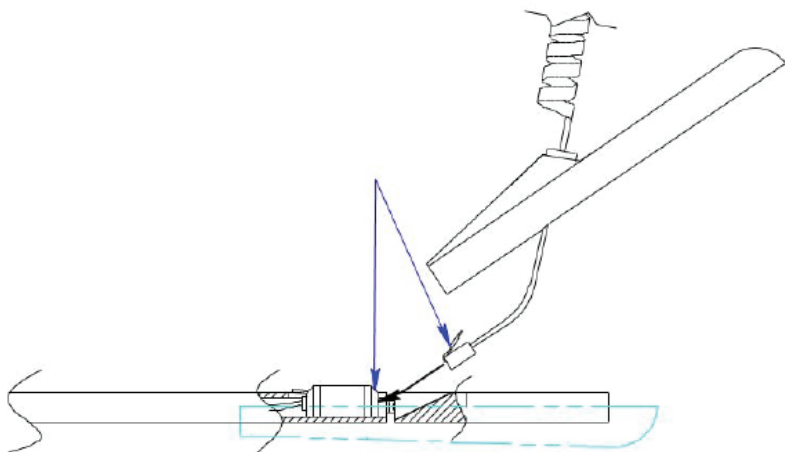

- **Step 6.** Carefully stow service loop and reassemble handle. See Step 1 for screw locations.

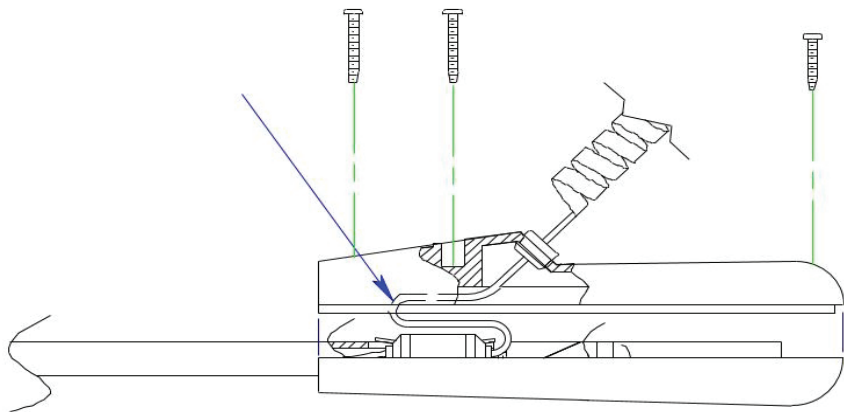

## REPAIR SERVICE

---

In the event of damage or failure, the Probe Head can be removed from the extrusion.

You have the option of sending in your entire Stack Probe or the Stack Probe Head. Your equipment will be repaired, calibrated, and returned promptly.


**NOTE:** Shipping costs for a complete Stack Probe is more than twice the cost to ship a Probe Head, due to the “oversized” length shipping companies charge.

If you would like to expedite the Probe repair, a replacement Probe Head can be ordered and shipped to you directly by Wagner. See Replacement Parts section for Part Numbers, which may be purchased from the factory or through your distributor.


Head removal is described below.

- **Step 1.** Lay the L722 Stack Probe on a flat work space with the coil cord facing upward. Remove the 6 screws fastening the handle half-shells together. Separate the two halves of the handle.


Remove 6 handle screws

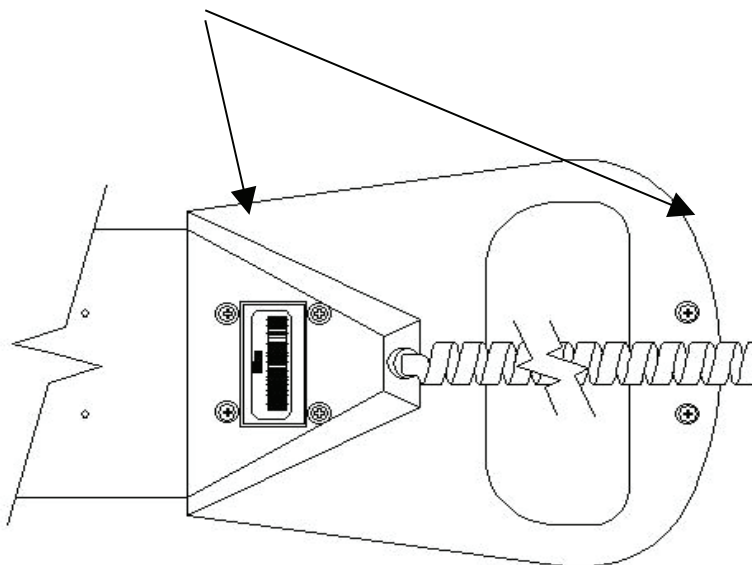

- **Step 2.** Disconnect the old cord from the coupler.

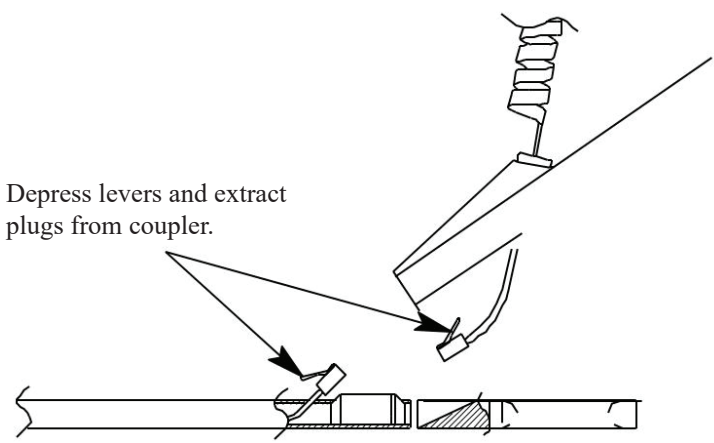

- **Step 2.** Loosen (2) inside extrusion screws, then remove (2) outside hinge dock screws. Gently pull the Probe Head and its attached cable from the extrusion.

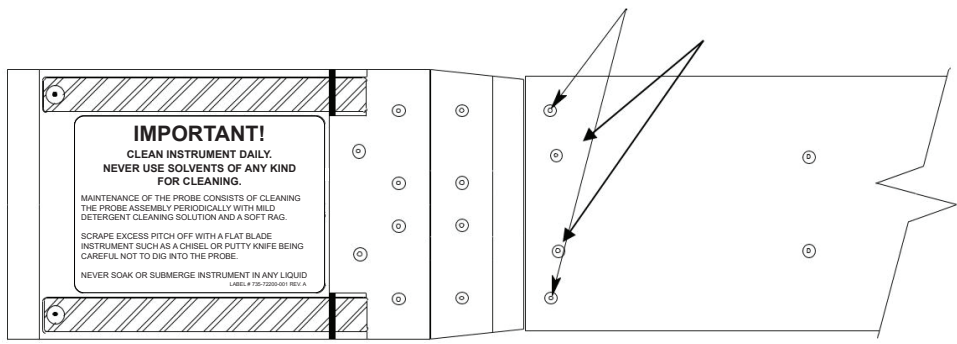

**Be sure to re-install Probe Head in reverse order.**

Please visit [www.wagnerrepairs.com](http://www.wagnerrepairs.com) and fill out the corresponding meter form and send it along with your Stack Probe or Probe Head to Wager Meters. All return information and pricing is on the form for your convenience.

## WARRANTY

---

Wagner Meters warrants this product against defects in material and workmanship for one (1) year from the date of purchase, subject to the following terms and conditions:

Wagner's liability under this warranty shall be limited, at Wagner's option, to the repair or replacement of this product or any part thereof, which is demonstrated to be defective. To exercise this warranty, the customer must phone, fax, or e-mail Wagner's Technical Service Department for an RMA (Return Materials Authorization) number and factory instructions for shipment. This limited warranty does not apply if accident, negligent handling, misuse, alteration, damage during shipment, or improper service have damaged the product. Wagner Meters shall in no event be liable for any breach of warranty or defect in this product, which exceeds the amount of the purchase price of the product. Wagner Meters shall not be liable for incidental or consequential damages for the breach of any express or implied warranty with respect to this product or its calibration.

With proper care and maintenance, as recommended in the manual, the meter should stay in calibration; however, because Wagner Meters has no control over the manner in which the unit will be used, it makes no warranty that the meter will stay in calibration for any specific period of time. Wagner Meters recommends purchasing a calibration verification block or returning the unit to the factory for diagnostic checkup and recalibration on the anniversary date of purchase, each year the meter is in service.

This warranty is in lieu of all other warranties whether oral or written, expressed or implied. Any implied warranties, including implied warranties of merchantability and fitness for a particular purpose, are excluded. Agents and employees of Wagner Meters are not authorized to make modifications to this warranty or additional warranties binding on Wagner Meters. Additional statements, whether oral or written (except written statements from an officer of Wagner Meters) do not constitute warranties and should not be relied upon by the customer.

This warranty is personal to the customer purchasing the product from Wagner Meters and is not transferable.


All products returned for repair must be accompanied by a Repair Order form found on our website at [www.wagnerrepairs.com](http://www.wagnerrepairs.com). Repair should be returned to the following address:

Wagner Meters  
326 Pine Grove Road  
Rogue River, Oregon 97537  
888-750-5867

## WARNINGS

---

### WARNING

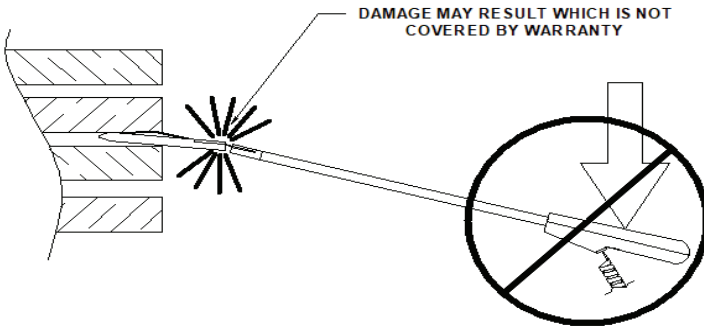

### CONDUCTIVE MATERIAL



THIS MATERIAL CAN CONDUCT HEAT AND ELECTRICITY

## NOTES

## NOTES



## NOTES



Wagner Meters  
326 Pine Grove Road  
Rogue River, OR 97537  
United States  
[info@wagnermeters.com](mailto:info@wagnermeters.com)

[WagnerMeters.com](http://WagnerMeters.com)  
(800) 505-1409

©Wagner Meters 2025

© Wagner Meters. All Rights Reserved Worldwide. No part of this publication may be reproduced, transmitted, transcribed, stored in a retrieval system, or translated into any other language in any form by any means without the express written permission of Wagner Meters.

For additional information, visit: [WagnerMeters.com](http://WagnerMeters.com)